



U of Chicago Fusion 2B-3R-6V-5YG-2UV

Cytometer:	FACSriaIII	User:	Administrator
Cytometer Name:	FACSriaIII	Institution:	N/A
Serial Number:	P65828200019	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	1/19/2018 12:43:41 PM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Blue Laser
(488nm)
FSC

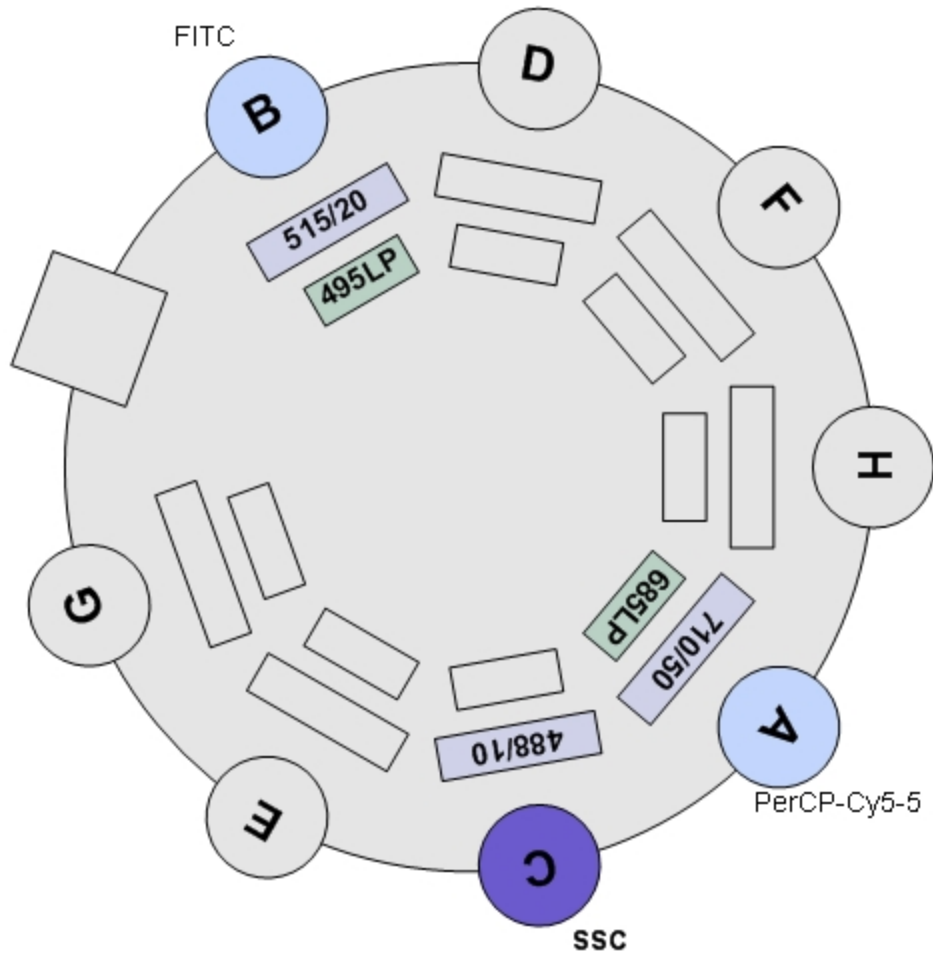


Red Laser
(640nm)

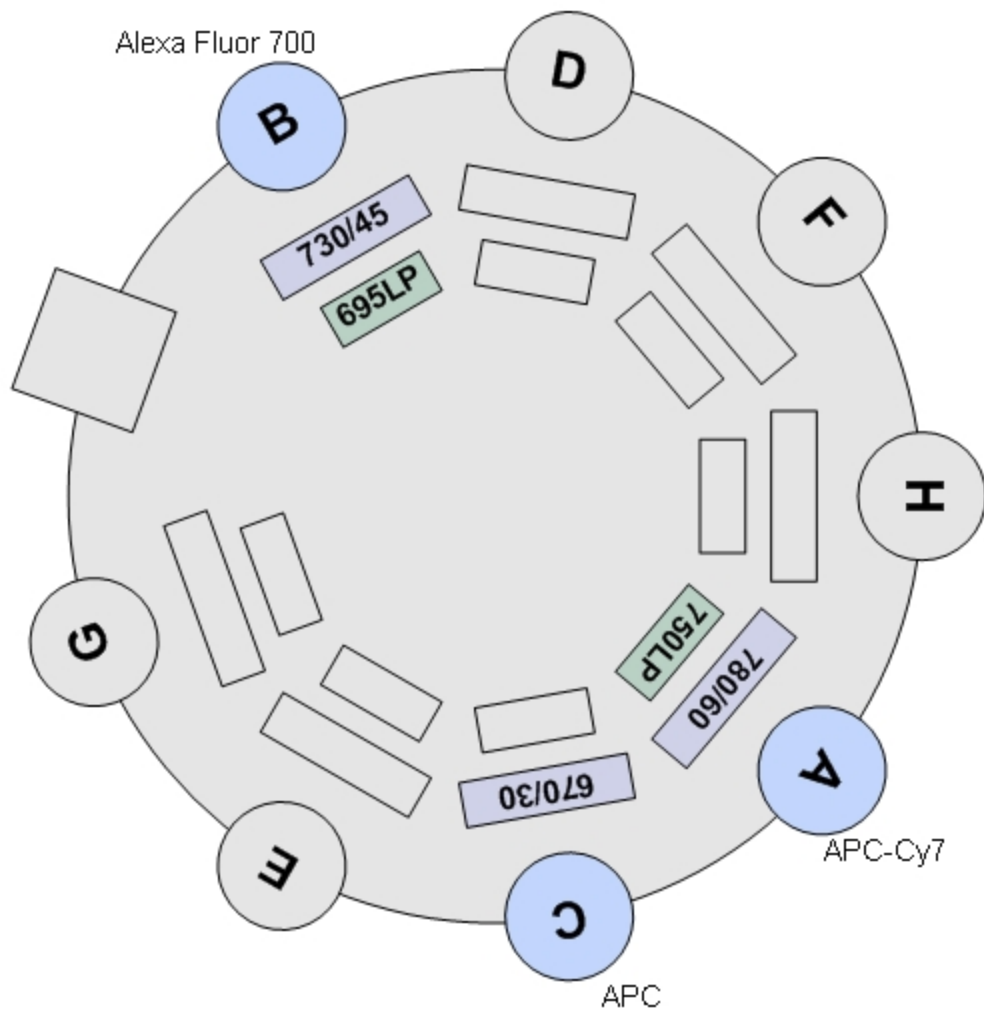


Violet Laser
(405nm)

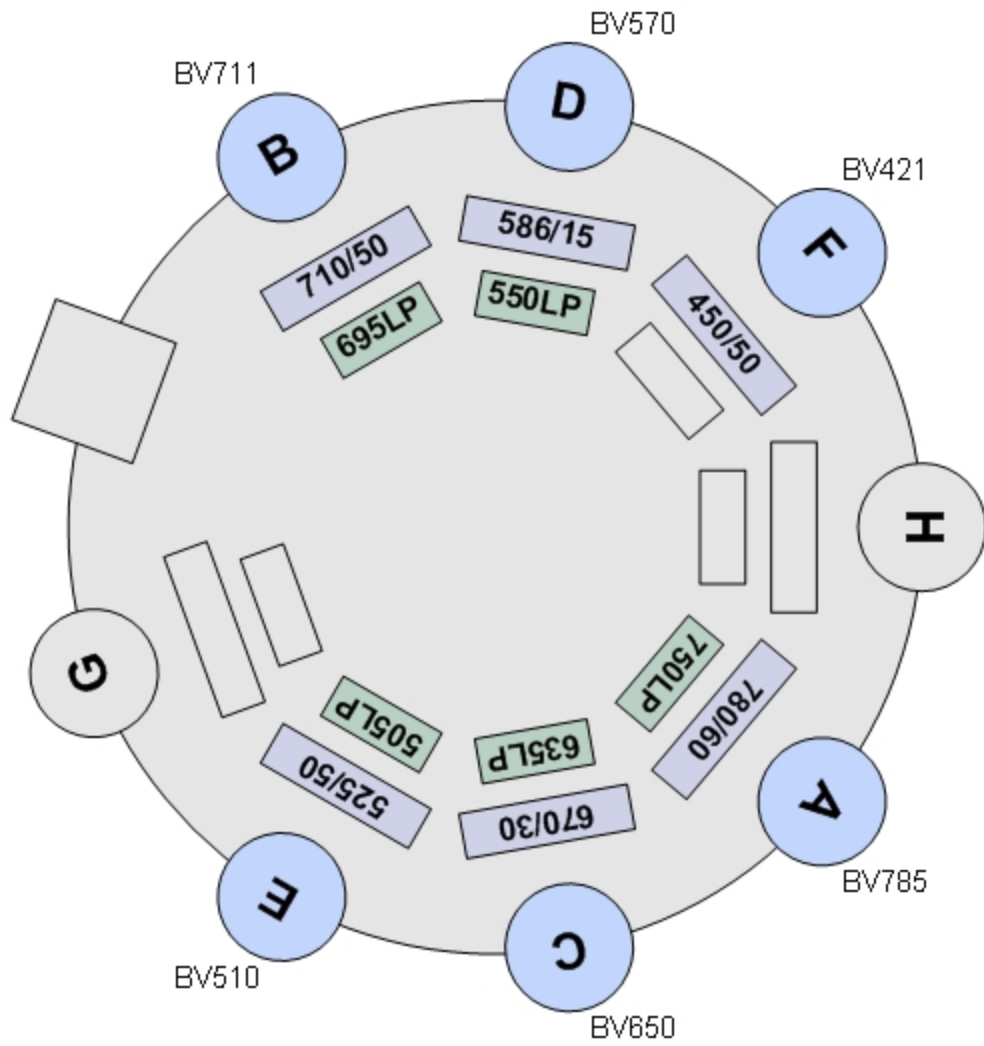

UV Laser
(355nm)

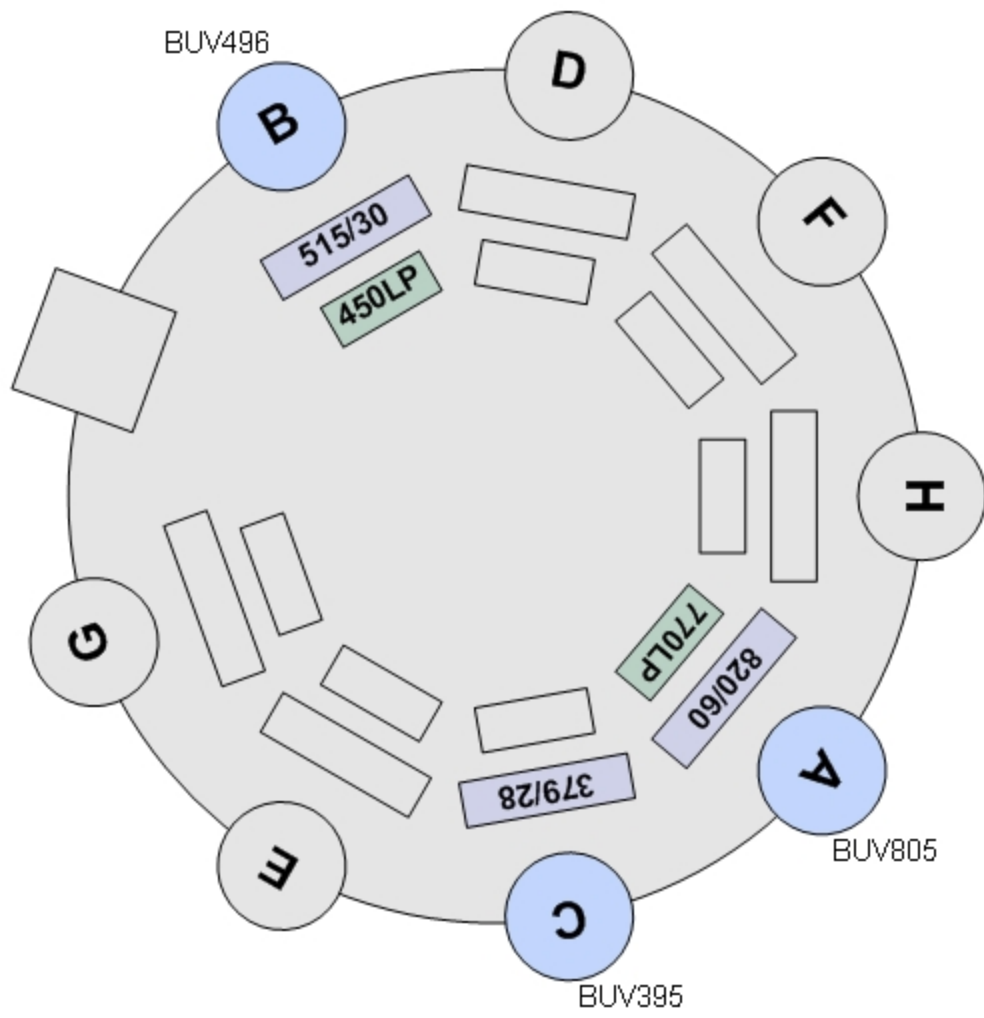

YG Laser
(561nm)

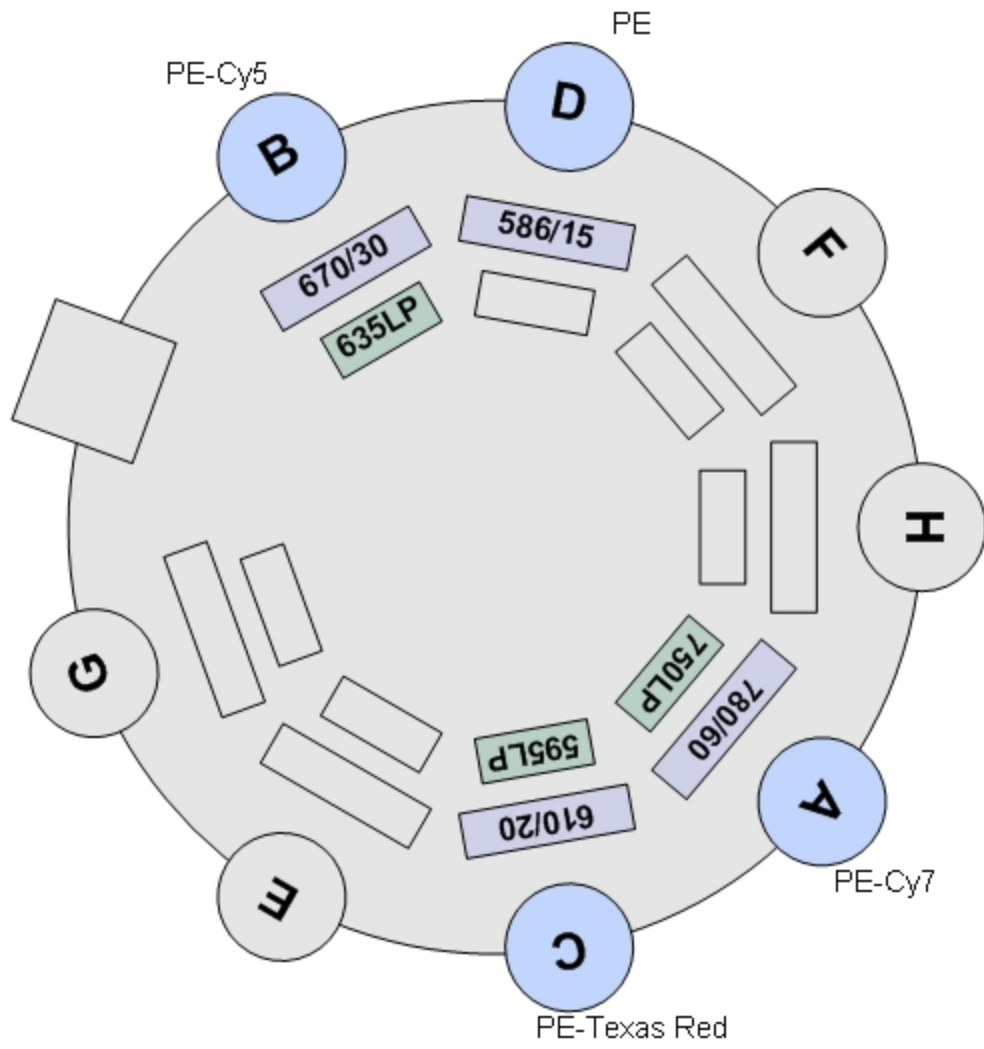

Comments: