



Use this configuration

Cytometer:	FACSAriaII	User:	Administrator
Cytometer Name:	FACSAriaII	Institution:	N/A
Serial Number:	P69500106	Software:	BD FACSDiva 8.0.1
Input Device:	Manual	Date:	8/7/2018 9:56:31 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Red Laser (633nm)

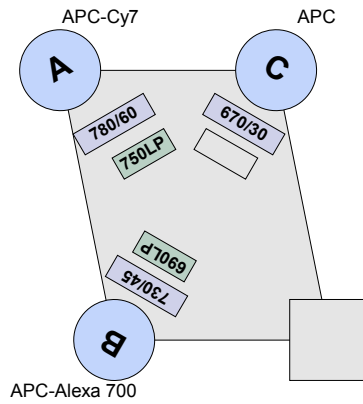


Blue Laser (488nm) FSC

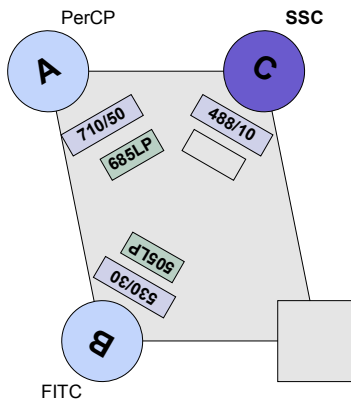

Violet Laser
(407nm)

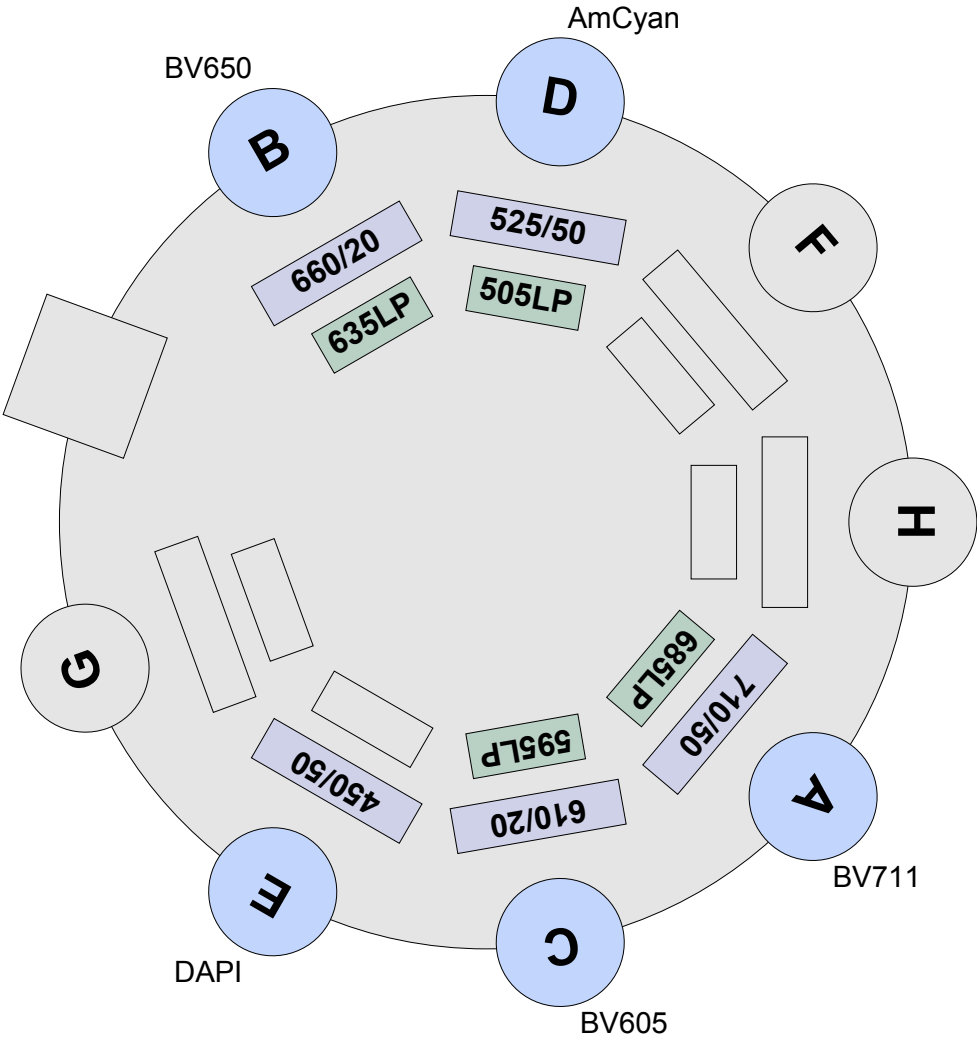

561 Yellow-Green Laser
(561nm)

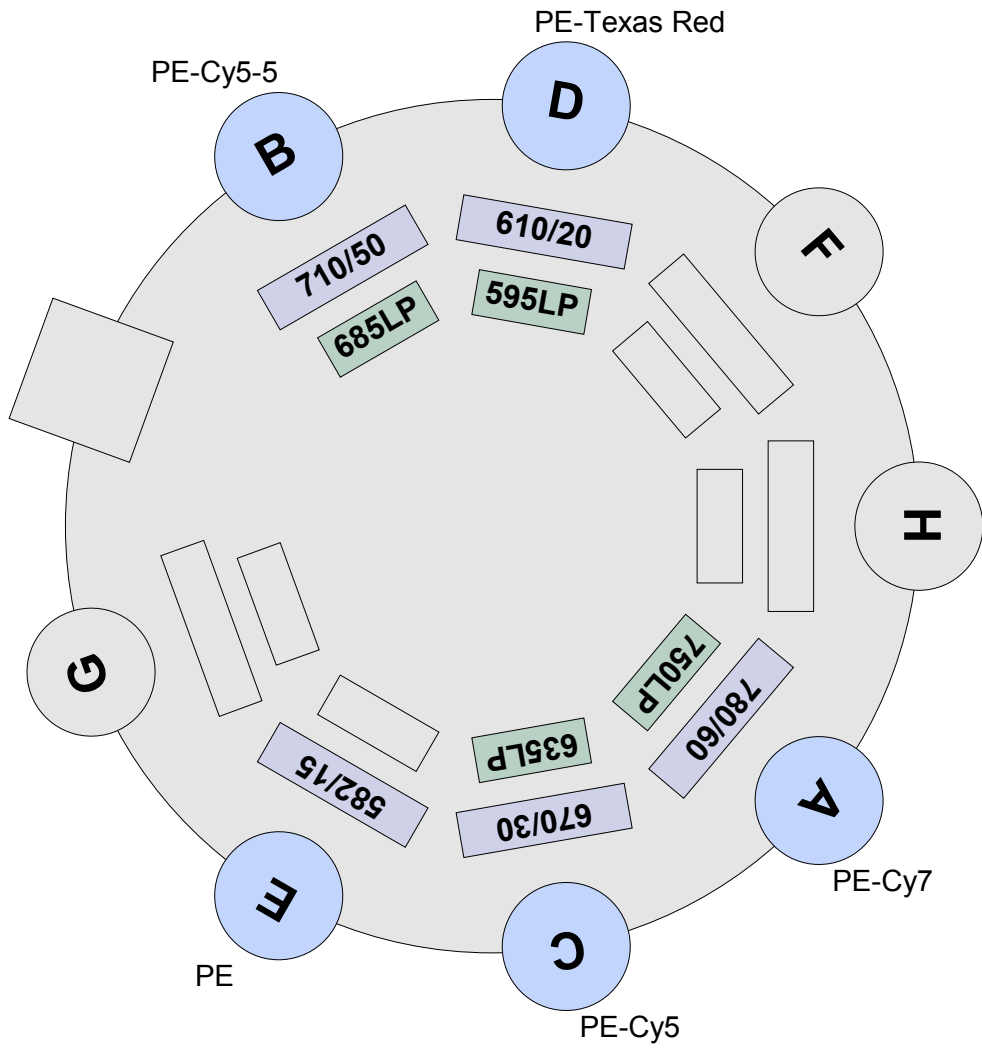

Comments: