



# Fortessa 4-15

Cytometer:	LSRFortessa	User:	Flowuser
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.2
Input Device:	Manual	Date:	1/19/2018 12:55:06 PM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

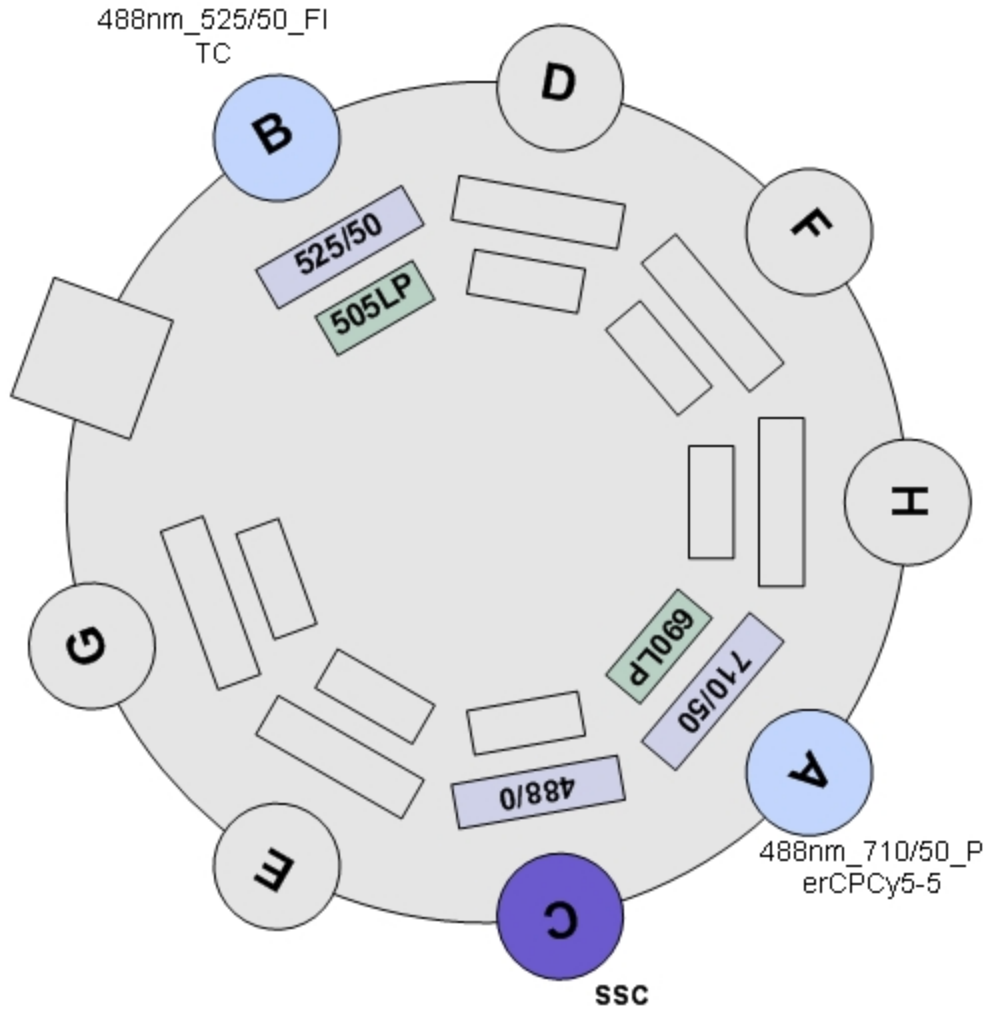


Red Laser  
(640nm)

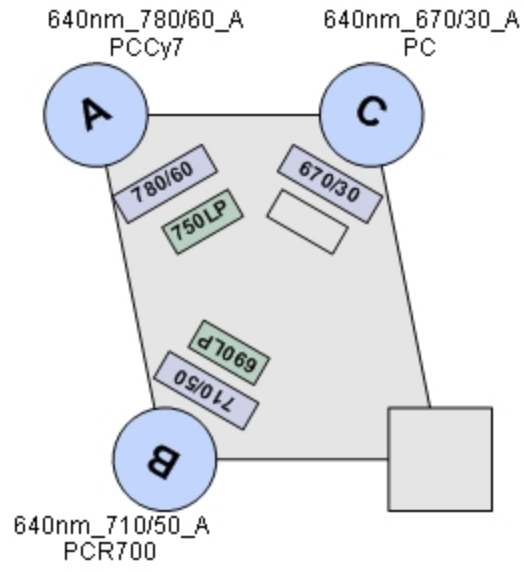

561 Yellow-Green Laser  
(561nm)

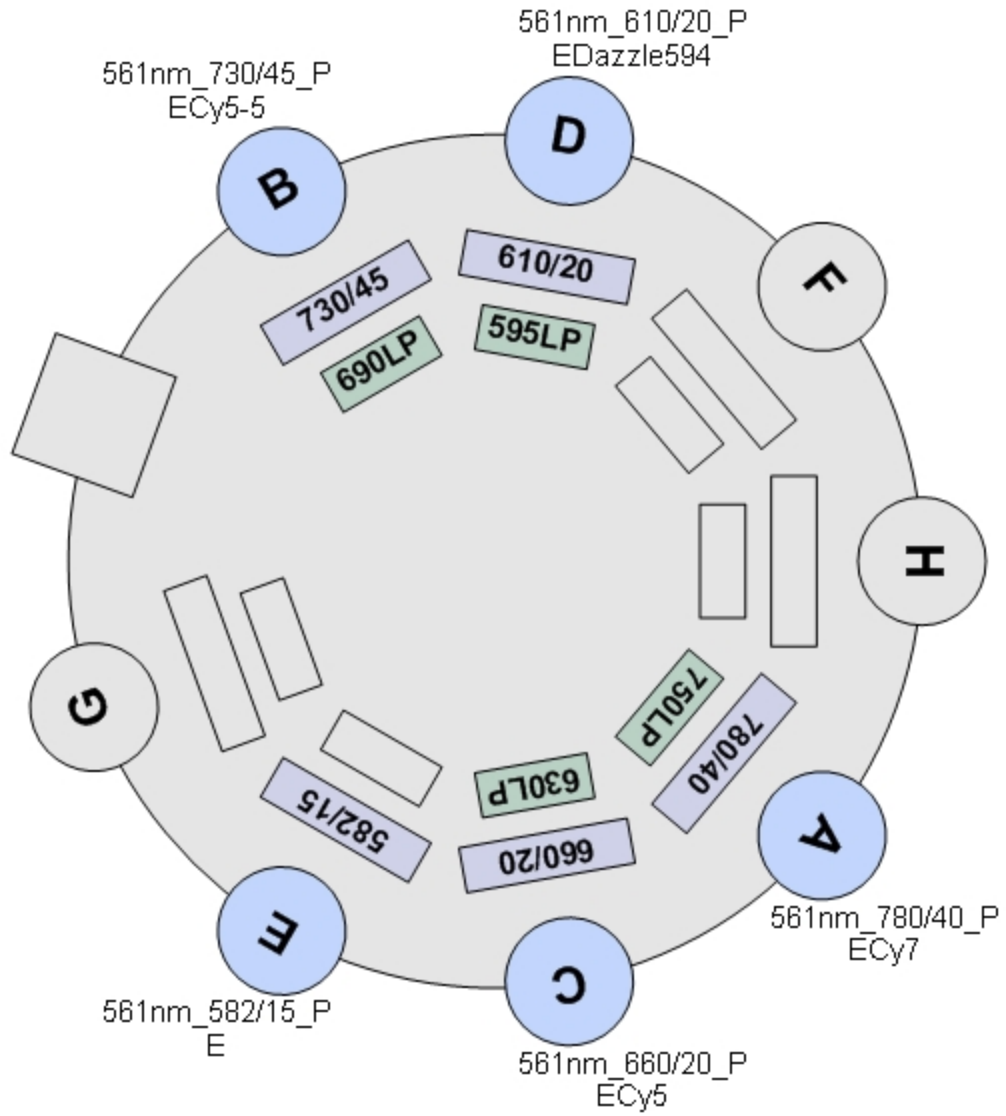

Violet Laser  
(405nm)

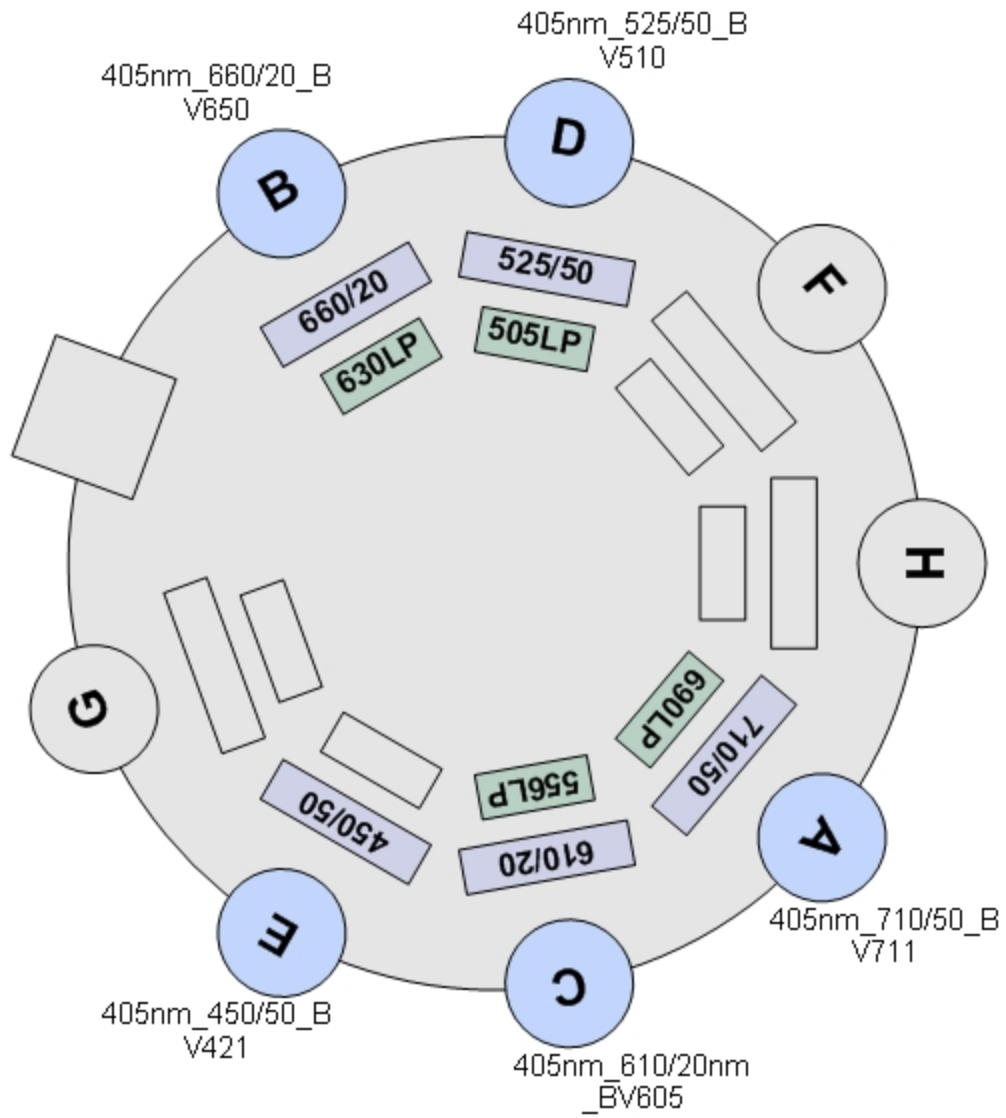

Comments: