

Comparative analysis of primer-probe sets for the laboratory confirmation of SARS-CoV-2

Yu Jin Jung^{1, †}, Gun-Soo Park^{1, 2, †}, Jun Hye Moon^{3, †}, Keunbon Ku¹, Seung-Hwa Beak^{1, 4}, Seil Kim^{1, 5}, Edmond Changkyun Park^{1, 6}, Daeui Park^{1, 4}, Jong-Hwan Lee¹, Cheol Woo Byeon³, Joong Jin Lee³, Jin-Soo Maeng^{1, 2}, Seong Jun Kim¹, Seung Il Kim^{1, 6}, Bum-Tae Kim¹, Min Jun Lee^{3, *}, and Hong Gi Kim^{1, *}

¹ *Center for Convergent Research of Emerging Virus Infection, Korea Research Institute of Chemical Technology, Daejeon 34114, Republic of Korea*

² *Research Group of Food Processing, Korea Food Research Institute, Wanju-gun, Jeollabuk-do 55365, Republic of Korea*

³ *Department of Molecular Diagnostics, WELLS BIO, INC, MagokJungang 8-ro 1-gil, Gangseo-gu, Seoul, Republic of Korea*

⁴ *Department of Predictive Toxicology, Korea Institute of Toxicology, Daejeon 34114, Republic of Korea*

⁵ *Division of Chemical and Medical Metrology, Center for Bioanalysis, Korea Research Institute of Standards and Science, Daejeon 34113, Republic of Korea*

⁶ *Research Center for Bioconvergence Analysis, Korea Basic Science Institute, Cheongju 28119, Republic of Korea*

† These authors contributed equally to this work.

* Corresponding authors: Hong Gi Kim (tenork@kriict.re.kr), and Min Jun Lee (mjlee@wellsbio.net)

Abstract

Coronavirus disease 2019 (COVID-19) is newly emerging human infectious diseases, which is caused by Severe Acute Respiratory Syndrome Coronavirus 2 (SARS-CoV-2, also previously known as 2019-nCoV). Within two months of the outbreak, more than 80,000 cases of COVID-19 have been confirmed worldwide. Since the human to human transmission occurred easily and the human infection is rapidly increasing, the sensitive and early diagnosis is essential to prevent the global outbreak. Recently, World Health Organization (WHO) announced various primer and probe sets for SARS-CoV-2 previously developed in China, Germany, Hong Kong, Japan, Thailand, and USA. In this study, we compared the ability to detect SARS-CoV-2 RNA among the seven primer-probe sets for N gene and the three primer-probe sets for Orf1 gene. The result of the comparative analysis represented that the '2019-nCoV_N2, N3' of USA and the 'ORF1ab' of China are the most sensitive primer-probe sets for N and Orf1 genes, respectively. Therefore, the appropriate combination from ORF1ab (China), 2019-nCoV_N2, N3 (USA), and NIID_2019-nCOV_N (Japan) sets should be selected for the sensitive and reliable laboratory confirmation of SARS-CoV-2.

Keywords: SARS-CoV-2, real-time qPCR, molecular diagnosis, 2019-nCoV, COVID-19

Introduction

Firstly informed to World Health Organization (WHO) on 31 December 2019, the current outbreak of Coronavirus Disease (COVID-19) involves 78,811 confirmed cases over 28 countries as of 23 February 2020 [1]. The majority of COVID-19 patients had pneumonia and showed symptoms include fever and cough [2, 3]. The genome sequence of causative novel coronavirus was shared through Global Initiative on Sharing All Influenza Data (GISAID) platform from 12 January 2020. The sequences of novel coronavirus (CoV) showed close similarity to that of severe acute respiratory syndrome-related coronaviruses (SARSr-CoV) and the virus uses ACE2 as the entry receptor like SARS-CoV [4-6]. The Coronavirus Study Group of the International Committee on Taxonomy of Viruses designated the virus as SARS-CoV-2 [7].

Molecular diagnosis of COVID-19 is currently carried out by one-step quantitative RT-PCR (qRT-PCR) targetting SARS-CoV-2 by which primers and probes being suggested by institutes of China, Germany, Hong Kong, Japan, Thailand, and USA were posted through WHO [8-10]. Clinical diagnosis methods including CT scan are also utilized to identify COVID-19 cases in Hubei province, China, from 13 February 2020 [11]. Although qRT-PCR assay served as a gold-standard method to detect respiratory infectious viruses such as SARS-CoV and MERS-CoV [12-15], current qRT-PCR assays targetting SARS-CoV-2 have some caveats. First, due to the high similarity of SARS-CoV-2 to SARS-CoV, primer-probe sets would cross-react. Second, the sensitivity of the assays may not enough to confirm suspicious patients in early time points after admission. Indeed, cases of positive CT scan results and negative RT-PCR results at initial presentation were reported [16]. The performance of molecular diagnosis might be dependent on primers, probes, and reagents. There have been no comparative results of the current qRT-PCR analysis for the molecular diagnosis of SARS-CoV-2.

In this present study, the qRT-PCR analysis was performed with previously reported primer-probe sets targetting RdRp/Orf1 and N region of SARS-CoV-2. This is the first comparative analysis of various primer-probe sets for the laboratory confirmation of SARS-CoV-2.

Materials and methods

Primer Information of qPCR

For the comparative analysis of laboratory confirmation for SARS-CoV-2, ten primer-probe sets were selected based on sequence information from the six different national institutions; the Centers for Disease Control and Prevention (CDC) (USA), Charité – Universitätsmedizin Berlin Institute of Virology (Germany), The University of Hong Kong (Hong Kong), National Institute of Infectious Disease, Department of virology III (Japan), China CDC (China), and National Institute of Health (Thailand). All of the DNA oligonucleotides were synthesized from Neoprobe (Daejeon, South Korea). The sequences of primer-probe sets and their locations at viral RNA (GenBank MN908947.3) were listed in Figure 1 and Table 1. Seven of the ten sets were derived from the N gene, and the other three sets were derived from Orf1 gene (RdRp, ORF 1b-Nsp14, and ORF 1-Nsp10). All DNA oligonucleotides were resuspended in nuclease-free water before use.

Viral RNA preparation

The infection experiments were performed in a biosafety level-3 (BSL-3) laboratory. African green monkey kidney Vero cells (ATCC CCL-81) were infected with a clinical isolate SARS-CoV-2 (BetaCoV/Korea/KCDC03/2020 provided from Korea CDC). After 72 h, the culture medium containing mature infectious virions (virus medium) was collected and viral RNA was isolated from the culture medium using the QIAamp viral RNA extraction Kit (Qiagen, Hilden, Germany) according to the manufacturer's instructions.

Preparation of in vitro transcribed RNA standard

The coding sequence of SARS-CoV-2 Envelope (E) protein, which cloned in pET21a plasmid was PCR amplified with T7 promoter primer (5' – AATACGACTCACTATAG – 3', Macrogen Inc., South Korea) and T7 terminator primer (5' – GCTAGTTATTGCTCAGCGG – 3', Macrogen) with AccuPower® PCR PreMix (-dye) kit (Bioneer Inc., South Korea). PCR product was then used as *in vitro* transcription template using MEGAscript™ T7 Transcription Kit (Invitrogen Inc., CA, USA). The copy number of *in vitro* transcribed RNA was calculated from

RNA concentration measured with Quantus™ Fluorometer (Promega Inc., WI, USA). Standardized amounts of *in vitro* produced RNA were used E primer and qRT-PCR to produce a standard curve.

Confirmatory qRT-PCR in RdRp and N

Extracted nucleic acid samples were tested for comparative analysis of SARS-CoV-2 by qRT-PCR. The Orf1 and N region of SARS-CoV-2 were used as the target sequences for SARS-CoV-2 specific gene. Briefly, 10 µL of purified viral RNA was amplified in a 20 µL reaction solution containing 1X 1 step RT-PCR mix (WELLS BIO INC., South Korea), and 300 nM of primers and probes for the target detection. The qRT-PCR was performed with a CFX 96 touch real-time PCR detection system (Bio-rad, Hercules, CA, USA). The qRT-PCR conditions applied in this study were programmed as follows: UNG incubation, RT incubation, and enzyme activation were serially performed at 25 °C for 2 minutes, at 55 °C for 10 minutes, at 94 °C for 3 minutes respectively. Thermal cycling was then performed at 94 °C for 15 seconds (denaturation), and at 60 °C for 30 seconds (annealing and amplification) for forty-five cycles.

Results and Discussion

Validation of qRT-PCR assay

The Ct value was not produced from negative control, indicating the reaction was done aseptically. The standard curve from E gene primer-probe set also showed the reaction was done accordingly. The R² value of the standard curve was 0.999 and the calculated amplification efficiency was 101.6%. These indicated that the qRT-PCR reaction was done in optimal condition. The viral concentration of supernatant and cell lysate was determined by E gene-based assay (Table 2).

RdRp/Orf1 Assays

The Ct value of RdRp_SARSr (Germany), HKU-ORF1b-nsp14 (Hong Kong), and ORF1ab (China) from low concentration (15 copies/reaction) were 43.00, 38.97, and 36.85, respectively (Table 2). The assay with RdRp_SARSr (Germany) set showed a positive signal from the single reaction of triplicate in the concentration of 15 copies/reaction. The assay with HKU-ORF1b-nsp14 (Hong Kong), and ORF1ab (China) sets showed positive signals in the concentration of 1.5 copies/reaction (data not shown). The R² value from RdRp_SARSr (Germany), HKU-ORF1b-nsp14 (Hong Kong), and ORF1ab (China) were 0.983, 0.997 and 0.997, respectively. The calculated amplification efficiency of RdRp_SARSr (Germany), HKU-ORF1b-nsp14 (Hong Kong), and ORF1ab (China) was 101.6%, 96.1%, and 109.8%, respectively. As a result, ORF1ab (China) set may be recommended for the laboratory confirmation of the RdRp/Orf1 gene.

N Assays

The Ct value of N (China), HKU-N (Hong Kong), NIID_2019-nCoV_N (Japan), WH-NIC N (Thailand), 2019-nCoV_N1, N2, and N3 (USA) from low concentration (15 copies/reaction) were 34.86, 35.43, 33.13, 38.13, 34.71, 33.14, and 33.09, respectively (Table 2). The Ct value of 2019-nCoV_N2, N3 (USA), and NIID_2019-nCoV_N (Japan) sets were similar to each other, and the sets could be regarded as the most sensitive sets. The moderately sensitive assay was based on 2019-nCoV_N1 (USA) and N (China). These sets had higher Ct value than the most

sensitive sets, however, the Ct values from low concentration (15 copies/ μ l) were still within the cut-off value (Ct <37). WH-NIC N (Thailand) set was less sensitive than other sets. The Ct value from low concentration (15 copies/ μ l) was close to the cut-off value (Ct <38). The R^2 value from of N (China), HKU-N (Hong Kong), NIID_2019-nCoV_N (Japan), WH-NIC N (Thailand), 2019-nCoV_N1, N2, and N3 (USA) were 0.989, 0.980, 0.987, 0.987, 0.986, 0.952, and 0.991, respectively. The calculated amplification efficiency of N (China), HKU-N (Hong Kong), NIID_2019-nCoV_N (Japan), WH-NIC N (Thailand), 2019-nCoV_N1, N2, and N3 (USA) were 89.4, 105.3, 100.7, 106.2, 95.2, 97.3, and 93.9, respectively. Therefore, 2019-nCoV_N2, N3 (USA), and NIID_2019-nCoV_N (Japan) sets should be beneficial for the laboratory confirmation of SARS-CoV-2 by qRT-PCR assay of N gene.

Conclusions

Various primer-probe sets were previously reported to detect SARS-CoV-2 by the qRT-PCR assay. The sensitivity of the assay may not enough to confirm suspicious patients in the early stage of SARS-CoV-2 infection. Nevertheless, there have been no comparative results of the current qRT-PCR analysis for the molecular diagnosis of SARS-CoV-2. In the present study, the first comparative analysis of various primer-probe sets targeting RdRp/Orf1 and N region of SARS-CoV-2 was performed by qRT-PCR for the laboratory confirmation. In the case of targeting RdRp/Orf1 region, ORF1ab (China) set might be the most sensitive than other sets. 2019-nCoV_N2, N3 (USA), and NIID_2019-nCoV_N (Japan) sets may be recommended for the sensitive qRT-PCR assay of N region. Therefore, the appropriate combination from ORF1ab (China), 2019-nCoV_N2, N3 (USA), and NIID_2019-nCoV_N (Japan) sets should be selected for the sensitive and reliable laboratory confirmation of SARS-CoV-2.

Acknowledgments

We appreciated to National Culture Collection for Pathogen of Korea CDC for providing clinical SARS-

CoV-2 isolate. This work was supported by National Research Council of Science and Technology grant by the Ministry of Science and ICT (Grant No. CRC-16-01-KRICT).

References

1. WHO *Coronavirus disease 2019 (COVID-19): Situation Report – 34*. 2020. DOI: https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200223-sitrep-34-covid-19.pdf?sfvrsn=44ff8fd3_2.
2. Guan, W.J., et al. *Clinical characteristics of 2019 novel coronavirus infection in China*. 2020. DOI: <https://doi.org/10.1101/2020.02.06.20020974>.
3. Huang, C., et al., *Clinical features of patients infected with 2019 novel coronavirus in Wuhan, China*. *Lancet*, 2020. **395**(10223): p. 497-506.
4. Wu, F., et al., *A new coronavirus associated with human respiratory disease in China*. *Nature*, 2020.
5. Zhou, P., et al., *A pneumonia outbreak associated with a new coronavirus of probable bat origin*. *Nature*, 2020.
6. Zhu, N., et al., *A Novel Coronavirus from Patients with Pneumonia in China, 2019*. *N Engl J Med*, 2020. **382**(8): p. 727-733.
7. Gorbalenya, A.E., et al. *Severe acute respiratory syndrome-related coronavirus: The species and its viruses – a statement of the Coronavirus Study Group*. 2020. DOI: <https://doi.org/10.1101/2020.02.07.937862>.
8. WHO *Coronavirus disease (COVID-19) technical guidance: Laboratory testing for 2019-nCoV in humans*. 2020. DOI: <https://www.who.int/emergencies/diseases/novel-coronavirus-2019/technical-guidance/laboratory-guidance>.
9. Chu, D.K.W., et al., *Molecular Diagnosis of a Novel Coronavirus (2019-nCoV) Causing an Outbreak of Pneumonia*. *Clin Chem*, 2020.
10. Corman, V.M., et al., *Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR*. *Euro Surveill*, 2020. **25**(3).
11. WHO *Coronavirus disease 2019 (COVID-19): Situation Report – 28*. 2020. DOI: [https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200217-sitrep-28-covid-](https://www.who.int/docs/default-source/coronaviruse/situation-reports/20200217-sitrep-28-covid-19.pdf?sfvrsn=44ff8fd3_2)

[19.pdf?sfvrsn=a19cf2ad_2](#).

12. Drosten, C., et al., *Identification of a novel coronavirus in patients with severe acute respiratory syndrome*. N Engl J Med, 2003. **348**(20): p. 1967-76.
13. Poon, L.L., et al., *A one step quantitative RT-PCR for detection of SARS coronavirus with an internal control for PCR inhibitors*. J Clin Virol, 2004. **30**(3): p. 214-7.
14. Corman, V.M., et al., *Assays for laboratory confirmation of novel human coronavirus (hCoV-EMC) infections*. Euro Surveill, 2012. **17**(49).
15. Corman, V.M., et al., *Detection of a novel human coronavirus by real-time reverse-transcription polymerase chain reaction*. Euro Surveill, 2012. **17**(39).
16. Xie, X., et al., *Chest CT for Typical 2019-nCoV Pneumonia: Relationship to Negative RT-PCR Testing*. Radiology, 2020: p. 200343.
17. China_CDC *Specific primers and probes for detection 2019 novel coronavirus*. 2020. DOI: http://ivdc.chinacdc.cn/kyjz/202001/t20200121_211337.html.
18. Nao, N., et al. *Detection of second case of 2019-nCoV infection in Japan*. 2020. DOI: https://www.who.int/docs/default-source/coronaviruse/method-niid-20200123-2.pdf?sfvrsn=fbf75320_7.
19. Health, T.M.o.P. *Diagnostic detection of Novel coronavirus 2019 by Real time RT- PCR*. 2020. DOI: https://www.who.int/docs/default-source/coronaviruse/conventional-rt-pcr-followed-by-sequencing-for-detection-of-ncov-rirl-nat-inst-health-t.pdf?sfvrsn=42271c6d_4.
20. US_CDC *2019-Novel Coronavirus (2019-nCoV) Real-time rRT-PCR Panel: Primers and Probes*. 2020. DOI: https://www.who.int/docs/default-source/coronaviruse/uscdcr-rt-pcr-panel-primer-probes.pdf?sfvrsn=fa29cb4b_2.

Figure and Tables

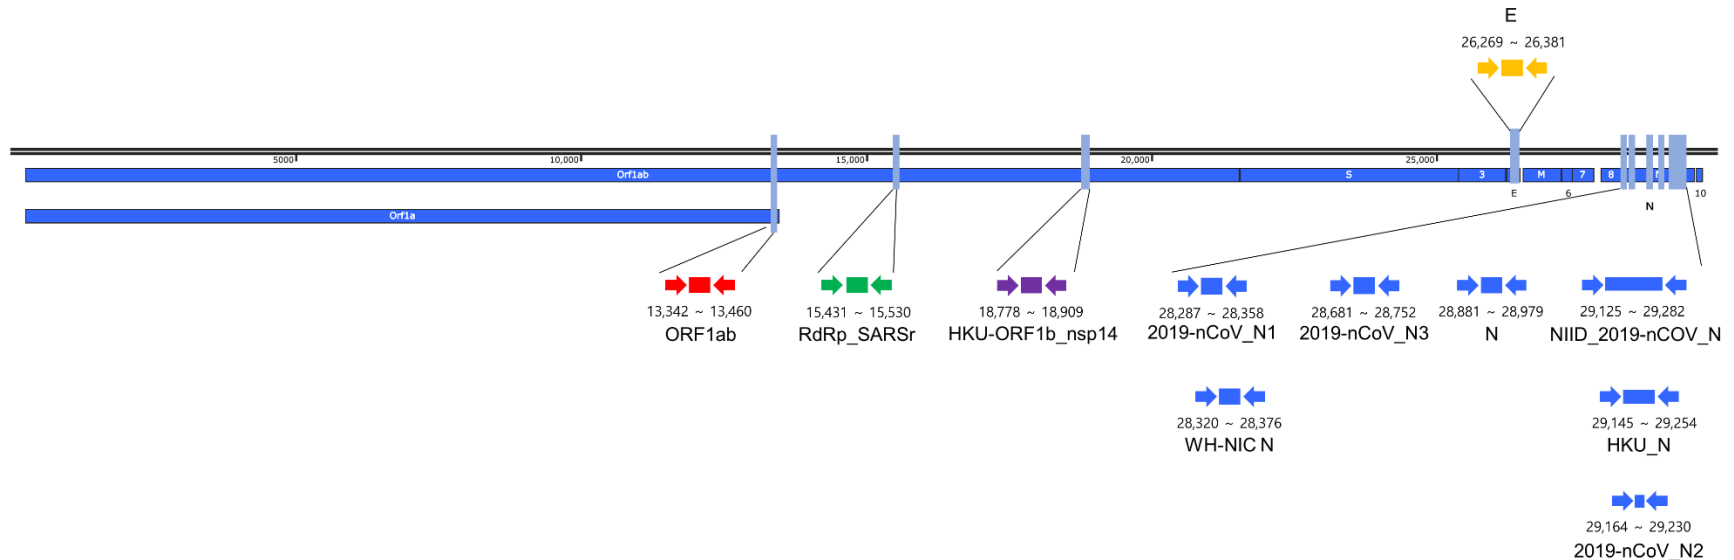


Figure 1. Relative positions of qRT-PCR primer-probe set on the SARS-CoV-2. The target genes and sequences of primers were searched from WHO website (<http://www.who.int>). The number below amplicons are genome positions according to SARS-CoV-2, GenBank MN908947.3. The sets were published by China CDC (Orf1ab and N), Charité – universitätsmedizin berlin institute of virology in Germany (RdRp_SARSr and E), the University of Hong Kong (HKU-ORF1b_nsp14 and HKU-N), USA CDC (2019-nCoV_N1, N2, and N3), National Institute of Health in Thailand (WH-NIC N), and National Institute of Infectious Disease in Japan (NIID_2019-nCoV_N). Orf1: open reading frame 1; RdRp: RNA-dependent RNA polymerase gene; Nsp14: non-structural protein 14 gene; S: spike protein gene; E: envelop protein gene, N: nucleocapsid protein gene

Table 1. Information of primers and probes analyzed in the study

Target	Country	Name	Type	Sequence (5' → 3')	Position	Reference
N	China	N-F	F	GGG GAA CTT CTC CTG CTA GAA T	28881 - 28902	[17]
		N-R	R	CAG ACA TTT TGC TCT CAA GCT G	28958 - 28979	
		N-P	P	TTG CTG CTG CTT GAC AGA TT	28934 - 28953	
	Hong Kong	HKU-NF	F	TAA TCA GAC AAG GAA CTG ATT A	29145 - 29166	[9]
		HKU-NR	R	CGA AGG TGT GAC TTC CAT G	29235 - 29254	
		HKU-NP	P	GCA AAT TGT GCA ATT TGC GG	29177 - 29196	
	Japan	NIID_2019-nCoV_N_F2	F	AAA TTT TGG GGA CCA GGA AC	29125 - 29144	[18]
		NIID_2019-nCoV_N_R2	R	TGG CAG CTG TGT AGG TCA AC	29263 - 29282	
		NIID_2019-nCoV_N_P2	P	ATG TCG CGC ATT GGC ATG GA	29222 - 29241	
	Thailand	WH-NIC N-F	F	CGT TTG GTG GAC CCT CAG AT	28320 - 28339	[19]
		WH-NIC N-R	R	CCC CAC TGC GTT CTC CAT T	28358 - 28376	
		WH-NIC N-P	P	CAA CTG GCA GTA ACC A	28341 - 28356	
	USA	2019-nCoV_N1-F	F	GAC CCC AAA ATC AGC GAA AT	28287 - 28306	[20]
		2019-nCoV_N1-R	R	TCT GGT TAC TGC CAG TTG AAT CTG	28335 - 28358	
		2019-nCoV_N1-P	P	ACC CCG CAT TAC GTT TGG TGG ACC	28309 - 28332	
		2019-nCoV_N2-F	F	TTA CAA ACA TTG GCC GCA AA	29164 - 29183	
		2019-nCoV_N2-R	R	GCG CGA CAT TCC GAA GAA	29213 - 29230	
		2019-nCoV_N2-P	P	ACA ATT TGC CCC CAG CGC TTC AG	29188 - 29210	
		2019-nCoV_N3-F	F	GGG AGC CTT GAA TAC ACC AAA A	28681 - 28702	
		2019-nCoV_N3-R	R	TGT AGC ACG ATT GCA GCA TTG	28732 - 28752	
	2019-nCoV_N3-P	P	AYC ACA TTG GCA CCC GCA ATC CTG	28704 - 28727		
RdRp/Orf1	China	ORF1ab-F	F	CCC TGT GGG TTT TAC ACT TAA	13342 - 13362	[17]
		ORF1ab-R	R	ACG ATT GTG CAT CAG CTG A	13442 - 13460	
		ORF1ab-P	P	CCG TCT GCG GTA TGT GGA AAG GTT ATG G	13377 - 13404	
	Germany	RdRp_SARSr-F	F	GTG ARA TGG TCA TGT GTG GCG G	15431 - 15452	[10]
		RdRp_SARSr-R	R	CAR ATG TTA AAS ACA CTA TTA GCA TA	15505 - 15530	
		RdRp_SARSr-P2	P	CAG GTG GAA CCT CAT CAG GAG ATG C	15470 - 15494	
	Hong Kong	HKU-ORF1b-nsp14F	F	TGG GGY TTT ACR GGT AAC CT	18778 - 18797	[9]
		HKU-ORF1b-nsp14R	R	AAC RCG CTT AAC AAA GCA CTC	18889 - 18909	
		HKU-ORF1b-nsp14P	P	TAG TTG TGA TGC WAT CAT GAC TAG	18849 - 18872	

Table 2. Comparative analysis of Ct values obtained by employing each primer-probe set

Target	Country	Name	Ct value			
			1.5×10^4 copies	1.5×10^3 copies	1.5×10^2 copies	1.5×10^1 copies
N	China	N	24.01	26.96	30.46	34.86
	Hong Kong	HKU-N	26.00	29.45	33.17	35.43
	Japan	NIID_2019-nCoV_N	23.09	26.56	29.5	33.13
	Thailand	WH-NIC N	28.64	31.89	35.26	38.13
	USA	2019-nCoV_N1	24.25	27.50	30.57	34.71
		2019-nCoV_N2	22.88	26.12	29.26	33.14
		2019-nCoV_N3	22.64	26.01	29.42	33.09
RdRp/Orf1	China	ORF1ab	27.33	30.33	33.61	36.85
	Germany	RdRp_SARSr	31.89	35.14	38.57	-*
	Hong Kong	HKU-ORF1b-nsp14	29.04	32.03	35.33	38.97

* The assay with RdRp_SARSr (Germany) set showed a positive signal (43.00) from the single reaction of triplicate.